

6050-4 3332F

USB PD 4 Channel ATE Test System



Basic version

Standard version

Value version

Complete version

Feature

- Can test 4 UUT at the same time to improve test efficiency and save test time and cost
- Select the required device configuration version (Basic / Standard / Value / Complete version) according to product testing requirements
- In addition to supporting USB PD, also supports QC2.0 / QC3.0 / PE+ / PE+2.0
- Highly cost-effective, fully functional modular design test system
- Operating environment of Windows 7 or higher (included)
- Open architecture software platform
 1. Support related hardware expansion
 2. Edit test item function
 3. Edit test program function
 4. Edit statistical analysis report function
 5. Online instrument control function
 6. User authorization settings
 7. Support Bar Code Reader

6050-4 (3332F) USB PD 4 Channel ATE Test System

USB PD Test items and equipment configuration table

Test items	Instrument Equipment							
	APS-7000 AC Source	99094 QC Controller	3332F DC Load	4032-PD Timing & Noise	4015A Power Meter	4013A Power Meter	PFR-100L OVP Source	5303 AVR
USB PD USB PD Performances								
USB PD Source / Sink Profile	✓	✓	✓					
USB PD Power Data Object (PDO)	✓	✓	✓					
Positive Voltage Transitions	✓	✓	✓	✓				
Negative Voltage Transitions	✓	✓	✓	✓				
Hard Reset	✓	✓	✓	✓				
USB Type C Cable unplug	✓	✓	✓	✓				
Output Performances								
Output Voltage	✓	✓	✓					
Output Current	✓	✓	✓					
Dynamic Load (Vpeak +/-)	✓	✓	✓	✓				
Average Efficiency	✓	✓	✓					
Ripple Voltage	✓	✓	✓	✓				
Input Characteristics								
Input RMS Current	✓	✓	✓		✓	✓		
Input Frequency	✓	✓	✓		✓	✓		
Input Power	✓	✓	✓		✓	✓		
No Load Power Consumption	✓	✓	✓		✓	✓		
Input Power Factor	✓	✓	✓		✓	✓		
Input Voltage Sag	✓	✓	✓	✓	✓	✓		
Current Harmonics	✓	✓	✓		✓			
Input Inrush Current	✓	✓	✓		✓	✓		✓
Regulation Tests								
Line Regulation	✓	✓	✓					
Load Regulation	✓	✓	✓					
Combine Regulation	✓	✓	✓					
Timing & Transient								
Turn ON (Set-Up) Time	✓	✓	✓	✓				
Turn OFF (Hold-Up) Time	✓	✓	✓	✓				
Rise Time	✓	✓	✓	✓				
Fall Time	✓	✓	✓	✓				
Protection Tests								
Short Circuit	✓	✓	✓					
OV Protection	✓	✓	✓				✓	
OC Protection	✓	✓	✓					
OP Protection	✓	✓	✓					


6050 USB PD 4 channel test system quick selection table

Test items	6050 USB PD 4 channel test system quick selection table			
	6050-4-A1 Basic version	6050-4-B1 Standard version	6050-4-C1 Value version	6050-4-D1 Compete version
USB PD USB PD Performances				
USB PD Source / Sink Profile	●	●	●	●
USB PD Power Data Object (PDO)	●	●	●	●
Positive Voltage Transitions		●	●	●
Negative Voltage Transitions		●	●	●
Hard Reset		●	●	●
USB Type C Cable unplug		●	●	●
Output Performances				
Output Voltage	●	●	●	●
Output Current	●	●	●	●
Dynamic Load (Vpeak +/-)		●	●	●
Average Efficiency	●	●	●	●
Ripple Voltage		●	●	●
Input Characteristics				
Input RMS Current	●	●	●	●
Input Frequency	●	●	●	●
Input Power	●	●	●	●
No Load Power Consumption	●	●	●	●
Input Power Factor	●	●	●	●
Input Voltage Sag	▲	●	●	●
Current Harmonics			●	●
Input Inrush Current				●
Regulation Tests				
Line Regulation	●	●	●	●
Load Regulation	●	●	●	●
Combine Regulation	●	●	●	●
Timing & Transient				
Turn ON (Set-Up) Time		●	●	●
Turn OFF (Hold-Up) Time		●	●	●
Rise Time		●	●	●
Fall Time		●	●	●
Protection Tests				
Short Circuit	●	●	●	●
OV Protection				●
OC Protection	●	●	●	●
OP Protection	●	●	●	●


△ Only provide Input Voltage Sag capability

6050-4-A1 Single Output USB PD basic verion 4 channel + AB switch test system Configuration is as shown in the table, just needs APS-7000 series AC Source, 3305F + 3332F series + 99094 Quick Charge Controller and 4013A Power Meter.

The basic version system configuration is shown below.

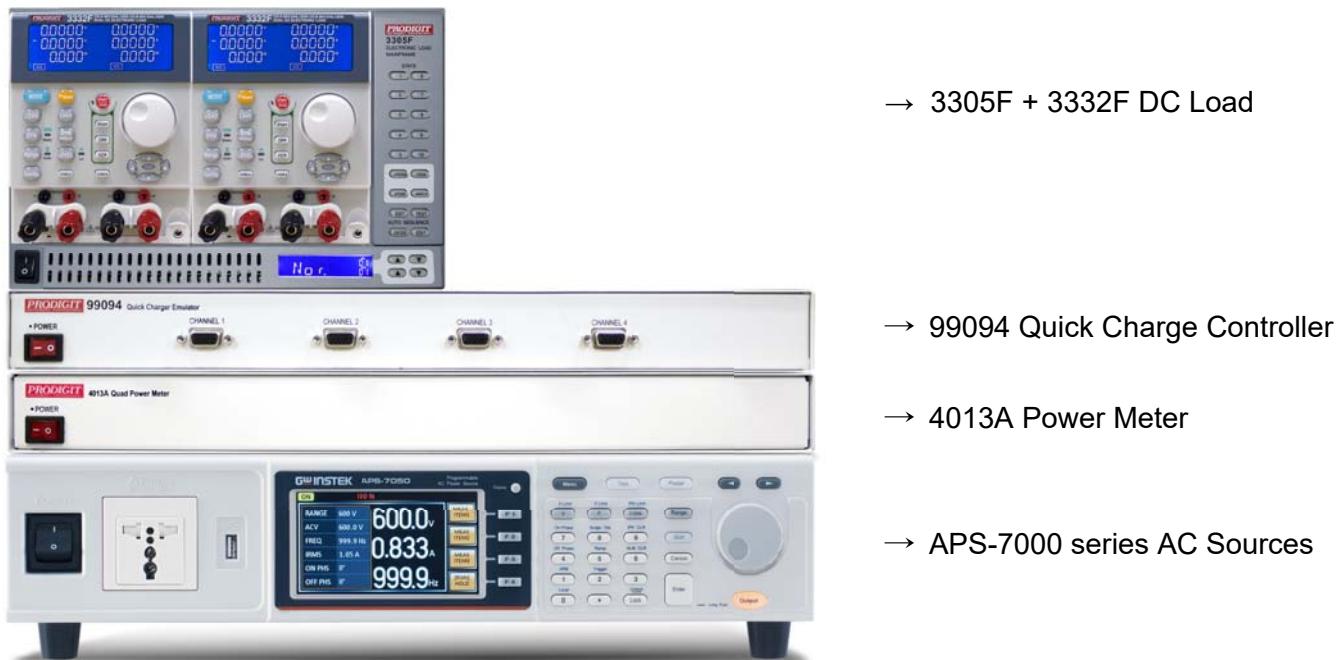

6050-4-A1 Basic version 4 channel test system block diagram

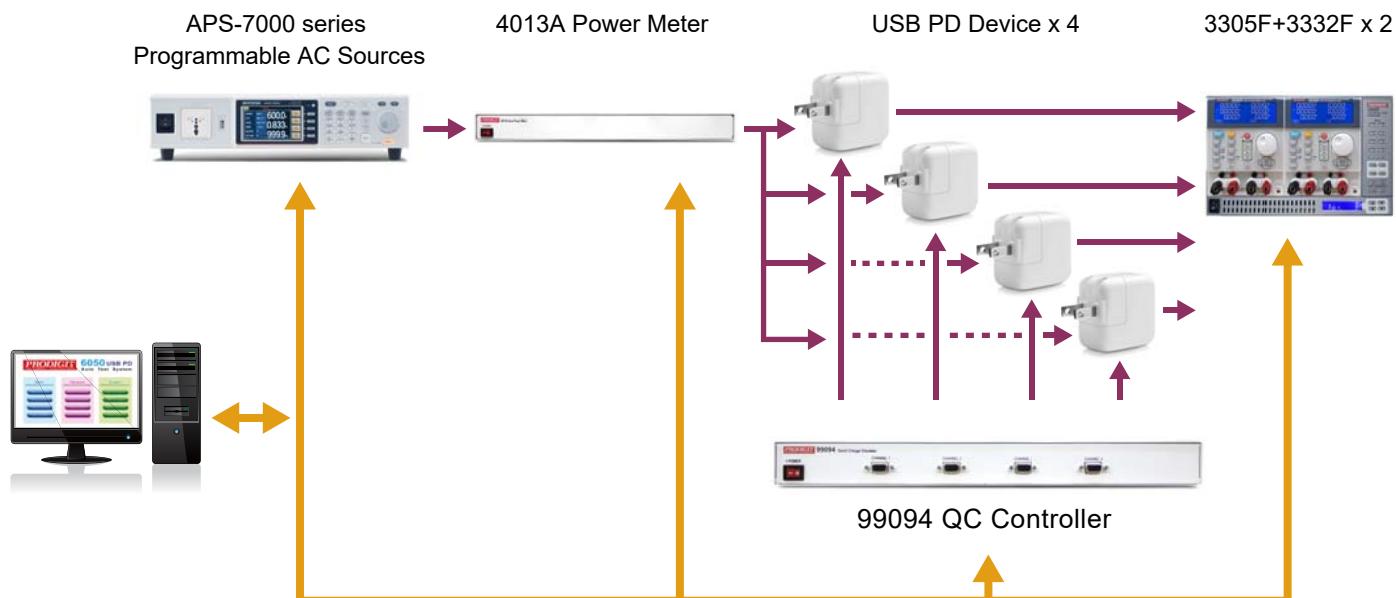

6050-4-A1 4 Channel Test System Configuration

6050-4-A1 Basic version 4 channel test system test items are as follows

USB PD Performances	Input Characteristics
USB PD Source / Sink Profile	Input RMS Current
USB PD Power Data Object (PDO)	Input Frequency
Output Performances	Input Power
Output Voltage	No Load Power Consumption
Output Current	Input Power Factor
Average Efficiency	
Regulation Tests	Protection Tests
Line Regulation	Short Circuit
Load Regulation	OC Protection
Combine Regulation	OP Protection

6050-4-A1 Basic version 4 channel test system equipment configuration table

Model	Quantity
APS-7000 Series Programmable Linear AC Power Sources	1
3305F 2CH Mainframe	1
3332F 80V/24A/120Wx 2 DC Load Module	2
99094 Quick Charge Controller (4 Channel)	1
4013A Power Meter (4 Channel)	1
6050 system software	1
System Controller (PC)	1
CP-104EL-A 1:4 High Speed RS-232 Card	1
Uport 1410 USB to RS-232 4 Port For Note Book	0
System Specifications (PC or Note Book)	
CPU	i5-3470(3.2GHz) or faster
SRAM	256KB
DRAM	4GB or higher
Hard Driver	500GB or higher
CD-ROM	40X or faster
Monitor	22"
KeyBoard	101 Keys
I/O	Mouse/Print Port
System Interface	RS-232
System I/O	1:4 or 1:8 High Speed RS-232 Card
O The system device should use this interface when using Note Book.	

OS : Windows 7.0 or latest version

6050-4-B1 Standard version 4 channel test system is consisted of basic version by adding 4032-PD Timing & Noise Meter x2 can increase USB PD characteristics and timing and transient testing.

The standard version system configuration is shown below.




→ 60104 + 4032-PD, 3332F, 3332F, 4032-PD

→ 99094 Quick Charge Controller

→ 4013A Power Meter

→ APS-7000 series AC Sources

6050-4-B1 Standard version 4 channel test system block diagram

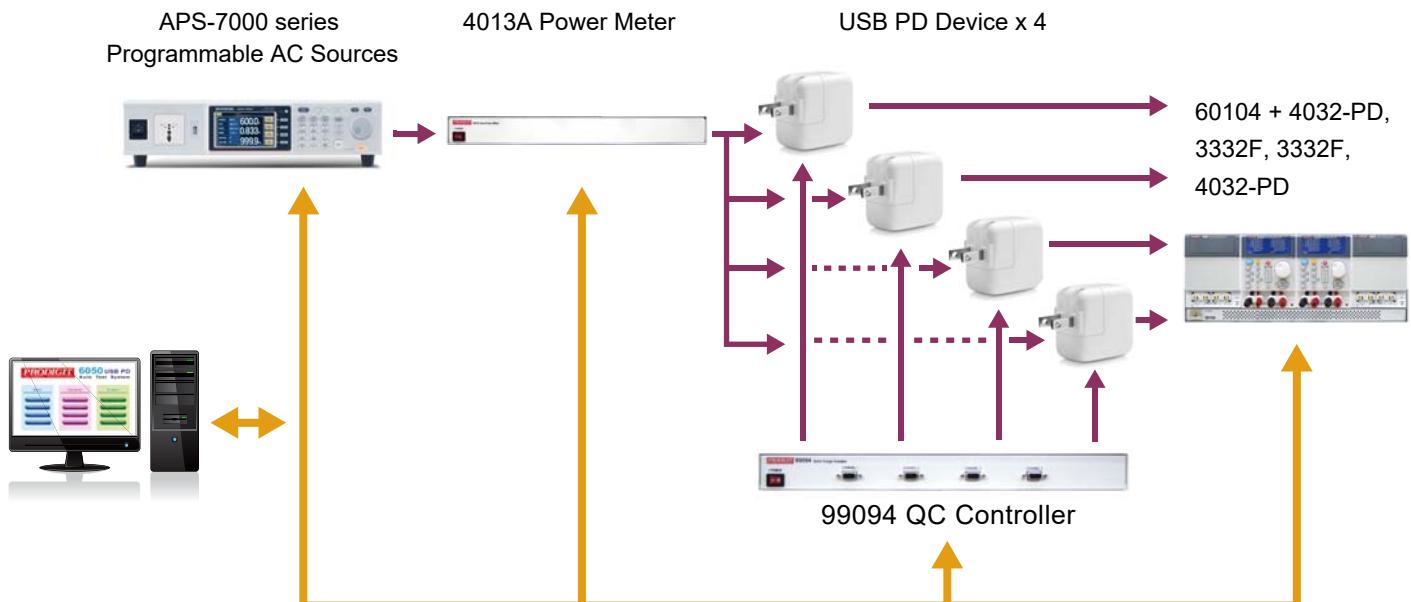

6050-4-B1 4 Channel Test System Configuration

6050-4-B1 Standard version 4 channel by adding 4034-PD and 99094 can increase the test items as shown in the block below.

USB PD Performances	Timing & Transient
Positive Voltage Transitions	Turn ON (Set-Up) Time
Negative Voltage Transitions	Turn OFF (Hold-Up) Time
Hard Reset	Rise Time
USB Type C Cable unplug	Fall Time
Output Performances	Input Characteristics
Dynamic Load (Vpeak +/-)	Input Voltage Sag
Ripple Voltage	

6050-4-B1 Standard version 4 channel test system equipment configuration table

Model	Quantity
APS-7000 Series Programmable Linear AC Power Sources	1
60104 4CH Mainframe; 4032-PD, 3332F,3332F,4032-PD	1
3332F 80V/24A/120Wx 2 DC Load Module	2
4032-PD Dual Timing & Noise Meter for PD	2
99094 Quick Charger Controller (4 Channel)	1
4013A Power Meter (4 Channel)	1
6050 system software	1
System Controller (PC)	1
CP-104EL-A 1:4 High Speed RS-232 Card	1
Uport 1410 USB to RS-232 4 Port For Note Book	0
System Specifications (PC or Note Book)	
CPU	i5-3470(3.2GHz) or faster
SRAM	256KB
DRAM	4GB or higher
Hard Driver	500GB or higher
CD-ROM	40X or faster
Monitor	22"
KeyBoard	101 Keys
I/O	Mouse / Print Port
System Interface	RS-232
System I/O	1:4 or 1:8 High Speed RS-232 Card
O The system device should use this interface when using Note Book.	

OS : Windows 7.0 or latest version

6050-4-C1 Value version (Standard version + Input current harmonic) 4 channel changing 4013A to 4015A power meter with Harmonic can increase the current harmonic Harmonics test. The value version system configuration is shown below.




→ 60104 + 4032-PD, 3332F, 3332F, 4032-PD

→ 99094 Quick Charge Controller

→ 4015A Power Meter with Harmonic

→ APS-7000 series AC Sources

6050-4-C1 Value version 4 channel test system block diagram

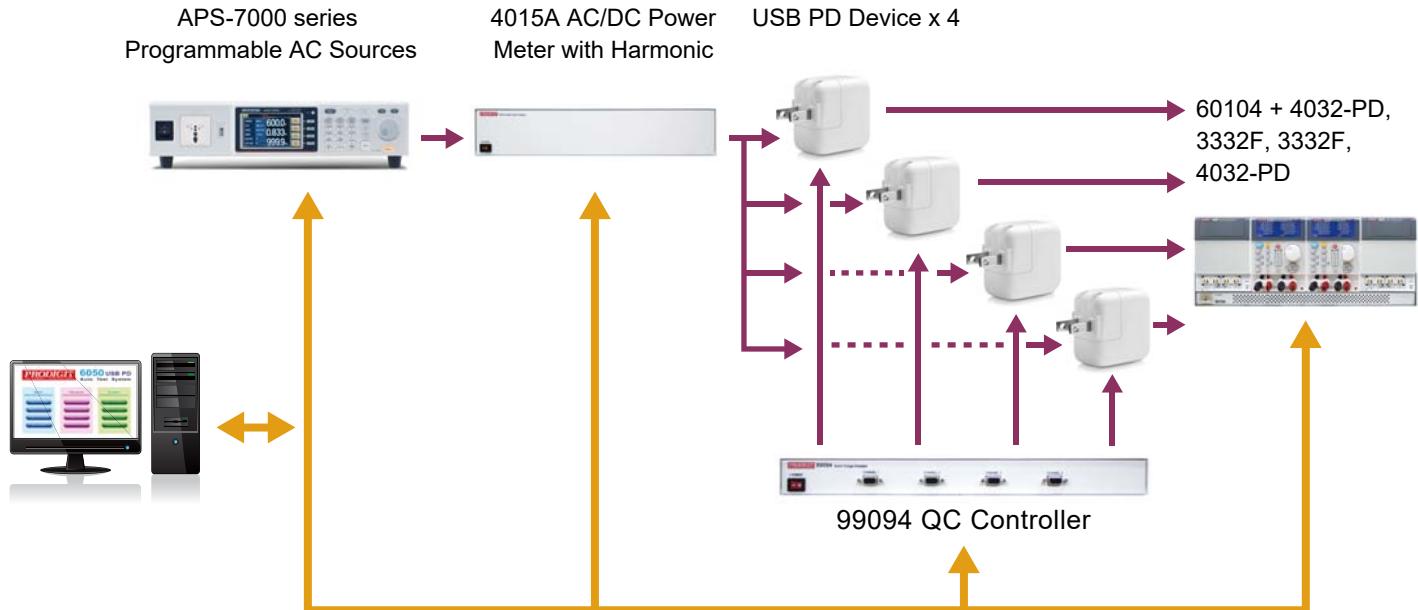

6050-4-C1 4 Channel Test System Configuration

6050-4-C1 Value version 4 channel test system : Changing 4013A to 4015A power meter can increase the test items as shown in the following green block

Input Characteristics
Current Harmonics

6050-4-C1 Value version 4 channel test system equipment configuration table

Model	Quantity
APS-7000 Series Programmable Linear AC Power Sources	1
60104 4CH Mainframe; 4032-PD, 3332F,3332F,4032-PD	1
3332F 80V/24A/120Wx 2 DC Load Module	2
4032-PD Dual Timing & Noise Meter for PD	2
4015A Power Meter with Harmonic (4 Channel)	1
99094 Quick Charger Controller (4 Channel)	1
6050 system software	1
System Controller (PC)	1
CP-104EL-A 1:4 High Speed RS-232 Card	1
Uport 1410 USB to RS-232 4 Port For Note Book	0
System Specifications (PC or Note Book)	
CPU	i5-3470(3.2GHz) or faster
SRAM	256KB
DRAM	4GB or higher
Hard Driver	500GB or higher
CD-ROM	40X or faster
Monitor	22"
KeyBoard	101 Keys
I/O	Mouse / Print Port
System Interface	RS-232
System I/O	1:4 or 1:8 High Speed RS-232 Card
O The system device should use this interface when using Note Book.	


OS : Windows 7.0 or latest version

6050-4-D1 Complete version (Standard version + Input Current Harmonics + Input Inrush Current)

4 channel test system : adding 5303 AVR and PFR-100L D.C. Power Supply to increase Input

Inrush Current and over voltage protection tests.

The Complete version system configuration is shown below.

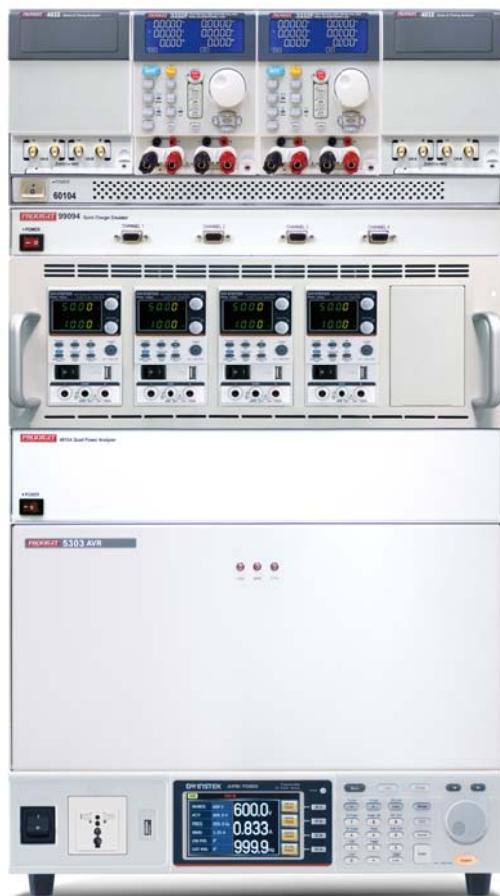

→ 60104 + 4032-PD, 3332F, 3332F, 4032-PD

→ 99094 Quick Charge Controller


→ PFR-100Lx4 D.C. Power Supply

→ 4015A Power Meter with Harmonic

→ 5303 AVR for Inrush Current

→ APS-7000 series AC Sources

6050-4-D Complete version 4 channel test system block diagram

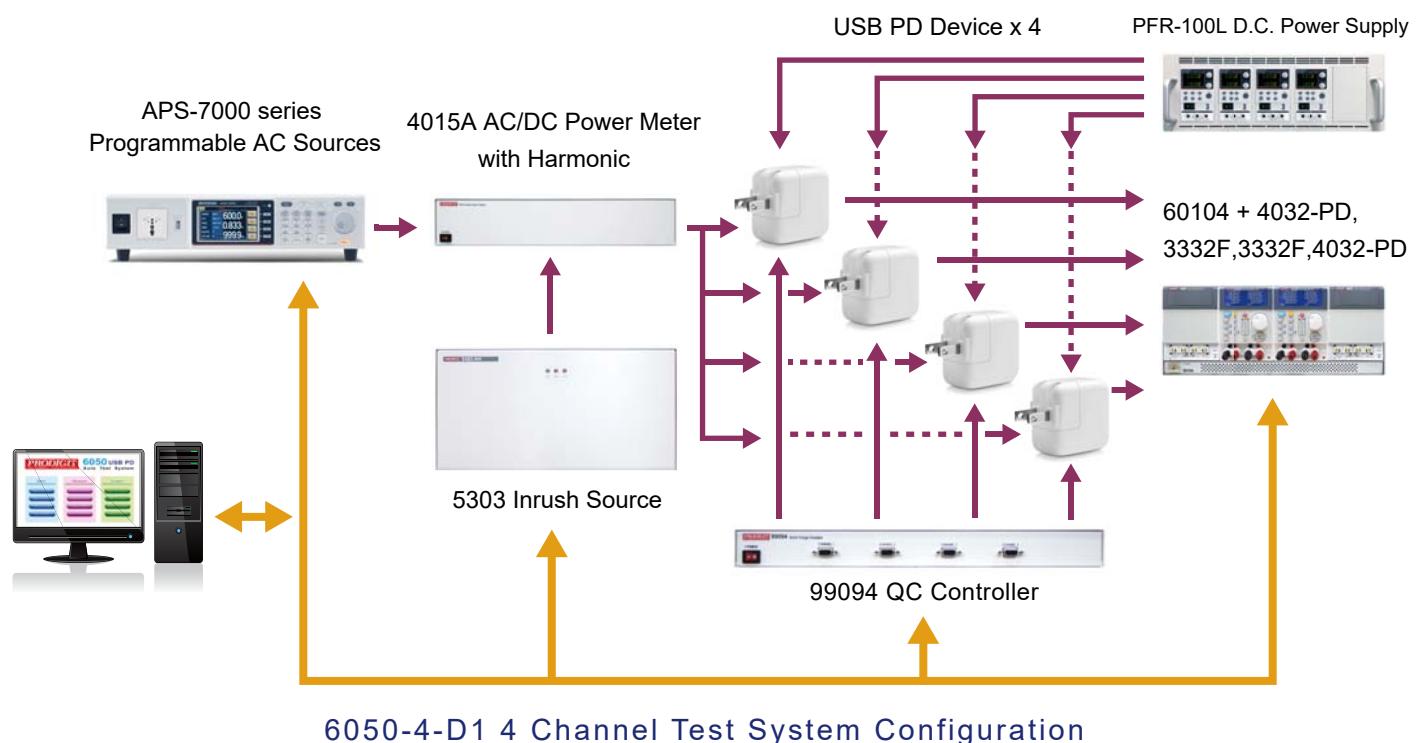

6050-4-D1 Complete version 4 channel test system by adding 5303 AVR and PFR-100L D.C. Power Supply can increase the test items

Input Characteristics	
Input Inrush Current	
Protection Tests	
OV Protection	

6050-4-D1 Complete version 4 channel test system equipment configuration table

Model	Quantity
APS-7000 Series Programmable Linear AC Power Sources	1
60104 4CH Mainframe; 4032-PD, 3332F,3332F,4032-PD	1
3332F 80V/24A/120Wx 2 DC Load Module	2
4032-PD Dual Timing & Noise Meter for PD	2
4015A Power Meter with Harmonic (4 Channel)	1
PFR-100L Fanless Multi-Range D.C. Power Supply	4
5303 3KVA AVR	1
99094 Quick Charger Controller (4 Channel)	1
6050 system software	1
System Controller (PC)	1
CP-104EL-A 1:4 High Speed RS-232 Card	1
Uport 1410 USB to RS-232 4 Port For Note Book	0
System Specifications (PC or Note Book)	
CPU	i5-3470(3.2GHz) or faster
SRAM	256KB
DRAM	4GB or higher
Hard Driver	500GB or higher
CD-ROM	40X or faster
Monitor	22"
KeyBoard	101 Keys
I/O	Mouse / Print Port
System Interface	RS-232
System I/O	1:4 or 1:8 High Speed RS-232 Card
O The system device should use this interface when using Note Book.	

OS : Windows 7.0 or latest version

All Equipment Functions and Specifications List

APS-7000 Series Programmable Linear AC Power Sources Suitable test item & Specifications

Model	APS-7000 Series Programmable Linear AC Power Sources							
Suitable Test Item								
1. Input RMS Current 2. Input Frequency 3. Input Power 4. No Load Power Consumption 5. Input Power Factor 6. Input Voltage Sag 7. Line Regulation 8. A voltage ON/OFF angle (0 ~ 360°) Can be programmed								
Specifications								
Power Rating	500VA	1000VA	2000VA	3000VA				
Voltage Rating	0 ~ 155Vrms, 0 ~ 310Vrms							
Current Rating	0~155Vrms 0~310Vrms	4.2A 2.1A	8.4A 4.2A	16.8A 8.4A				
Frequency	45 ~ 500 Hz							
Angle (ON/OFF)	0 ~ 359°							
PQT<IEC 61000-4-11>	DIP, Interupt, Variation							
MEASUREMENT								
ACV meter (Vrms)	0 ~ 155Vrms, 0 ~ 310Vrms, Auto							
Voltage (RMS)	Range	0.20~38.75Vrms;38.76~77.50Vrms;77.51~155.0Vrms;155.1~310.0Vrms						
	Resolution	0.01V at 0.00 ~ 99.99Vrms; 0.1V at 100.0 ~ 310.0Vrms						
	Accuracy *4	±(0.5% of reading + 2 counts)						
Frequency	Range	45 ~ 500Hz						
	Resolution	0.01Hz at 45Hz~99.99Hz ; 0.1Hz at 100Hz~500.0Hz						
	Accuracy	±0.1Hz						
Current (RMS)	Range	2.00 ~ 70.00mA ; 60.0 ~ 350.0mA ; 0.300 ~ 3.500A ; 3.00 ~ 17.5A	0.200 ~ 3.500A ; 3.00 ~ 35.00A					
	Resolution	0.01mA, 0.1mA, 0.001A, 0.01A	0.001A ; 0.01A					
	Accuracy	± (0.6% of reading+5 counts), 2.00~350.0mA ; ± (0.5% of reading+5 counts), 0.300~3.500A ; ± (0.5% of reading+3 counts), 3.000~17.50A	± (0.5% of reading + 5 counts) , 0.200 ~ 3.500A ± (0.5% of reading + 3 counts) , 3.00 ~ 35.00A					
Current (Peak)	Range	0.0 ~ 70.0A						
	Resolution	0.1A						
	Accuracy	± (1% of reading + 1 count)						
Power (W)	Resolution	0.01W, 0.1W, 1W	0.1W, 1W					
	Accuracy	± (0.6% of reading+5 counts), 0.20~99.99W ; ± (0.6% of reading+5 counts), 100.0~999.9W ; ± (0.6% of reading+2 counts), 1000~9999W	± (0.6% of reading + 5counts) , 0.2 ~ 999.9W ± (0.6% of reading + 2counts) , 1000 ~ 9999W					
Apparent (VA)	Resolution	0.01VA, 0.1VA, 1VA	0.1VA, 1VA					
	Accuracy	±(1% of reading+7 counts), 0.20~99.99VA ; ±(1% of reading+7 counts), 100.0~999.9V A ; ±(1% of reading+5 counts), 1000~9999VA	± (1% of reading + 7 counts) , 0.2 ~ 999.9VA ; ± (1% of reading + 5 counts) , 1000 ~ 9999VA					
Power Factor	Resolution	0.001						
	Accuracy	± (2% of reading + 2 counts)						
Frequency meter	45 ~ 500Hz							
Interface	RS-232							

Table 1 - Preferred test level and durations for voltage dips

Class ^a	Test level and durations for voltage dips(ts) (50 Hz/60 Hz)				
Class 1	Case-by-case according to the equipment requirements				
Class 2	0 % during 1/2 cycle	0 % during 1 cycle	70 % during 25/30 ^c cycles		
Class 3	0 % during 1/2 cycle	0 % during 1 cycle	40 % during 10/12 ^c cycles	70 % during 25/30 ^c cycles	80 % during 250/300 ^c cycles
Class X ^b	X	X	X	X	X

a Classes as per IEC 61000-2-4; see Annex B.
 b To be defined by product committee. For equipment connected directly or indirectly to the public network, the levels must not be less severe than Class 2.
 c "25/30 cycles" means "25 cycles for 50 Hz test" and "30 cycles for 60 Hz test"

Table 2 - Preferred test level and durations for short interruptions

Class ^a	Class ^a Test level and durations for short interruptions (ts) (50 Hz/60 Hz)
Class 1	Case-by-case according to the equipment requirements
Class 2	0 % during 250/300 ^c cycles
Class 3	0 % during 250/300 ^c cycles
Class X ^b	X

a Classes as per IEC 61000-2-4 ; see Annex B.
 b To be defined by product committee. For equipment connected directly or indirectly to the public network, the levels must not be less severe than Class 2.
 c "250/300 cycles" means "250 cycles for 50 Hz test" and "300 cycles for 60 Hz test"

Table 3 - Timing of short-term supply voltage variations

Voltage test level	Time for decreasing voltage (<i>t_d</i>)	Time at reduced voltage (<i>t_s</i>)	Time for increasing voltage (<i>t_i</i>) (50 Hz/60 Hz)
70%	Abrupt	1 cycle	25/30 ^b cycles
X ^a	X ^a	X ^a	X ^a
a To be defined by product committee.			
b "25/30 cycles" means "25 cycles for 50 Hz test" and "30 cycles for 60 Hz test".			

3332F DC E-Load List of Specification and applicable features

Model	3332F DC E-Load			
Applicable test function				
1. Output Voltage	5. Average Efficiency			
2. Output Current	6. Short Circuit			
3. Dynamic Load	7. OC Protection			
4. Efficiency	8. OP Protection			
Specifications				
Power	120W x 2			
Current	24A			
Voltage	80V			
Constant Current Mode				
Range	0 ~ 2.4A	0 ~ 24A		
Constant Resistance Mode				
Range	3.33Ω ~ 199.80KΩ	0.0333Ω ~ 3.33Ω		
Constant Voltage Mode				
Range	0 ~ 6V	0 ~ 80V		
Constant Power Mode				
Range	0 ~ 12W	0 ~ 120W		
Dynamic Mode				
Timing				
Thigh & Tlow	0.050 ~ 9.999 / 99.99 / 999.9 / 9999mS			
Resolution	0.001 / 0.01 / 0.1 / 1mS			
Slew rate	1.6 ~ 100mA/uS	16 ~ 1000mA/uS		
Accuracy	± (5% of Setting) ±10uS			
Measurement				
Voltage Read Back				
Range (5 Digital)	6V	81V		
Current Read Back				
Range (5 Digital)	2.4A	24A		
Resolution	0.0001A	0.001A		
Current Monitor	FULL SCALE 10V			
Current Programming Input	FULL SCALE 10V			
Programmable Short	BUILT-IN			
Load ON Voltage	0.1 ~ 25V			
Accuracy	1% of (Setting + Range)			
Load OFF Voltage	0 ~ 25V			
Accuracy	0.025% of (Setting + Range)			
Typical Short Resistance	0.02 Ω			
Maximum Short Current	30 A			
Operating range				
Temperature	0 ~ +40°C			
Humidity	20 ~ 85%rh			

4013A List of Specification and applicable features

Model	4013A Power Meter
No. of Input Channel	4
Applicable test function	
1. Input RMS Current	4. No Load Power Consumption
2. Input Frequency	5. Input Power Factor
3. Input Power	
Specifications	
ACV meter(Vrms)	30V / 300V
Resolution	16-bit
Accuracy	$\pm 0.5\%$ of (Reading + Range)
ACA meter(Arms)	20mA / 200mA / 2A / 20A / 200A(for Inrush)
Resolution	16-bit
Accuracy	$\pm 0.5\%$ of (Reading + Range) / $\pm 2\%$ of (Reading + Range) (for Inrush)
ACW meter	0.6W / 6W / 60W / 600W / 6000W
Resolution	32-bit
Accuracy	$\pm 0.5\%$ of (Reading + Range)
DCV meter	40V / 400V
Resolution	0.001V / 0.01V
Accuracy	$\pm 0.5\%$ of (Reading + Range)
DCA meter	20mA / 200mA / 2A / 20A / 200A(for Inrush)
Resolution	0.001mA / 0.01mA / 0.1mA / 1mA / 10mA(for Inrush)
Accuracy	$\pm 0.5\%$ of (Reading + Range) / $\pm 2\%$ of (Reading + Range) (for Inrush)
DCW meter	800mW / 8W / 80W / 800W / 8000W
Resolution	32-bit
Accuracy	$\pm 0.5\%$ of (Reading + Range)
PF meter	$\pm 0.01\sim 1.00$
Resolution	0.01
Accuracy	Corresponds to V and A, 1% of (Reading + Range)
Frequency meter	40~70 Hz
Resolution	0.1 Hz
Accuracy	± 0.1 Hz
Inrush Delay/Period	0~99.9ms/0.1~99.9s
Meter Meas. Rate Interval time	100ms / 200ms / 500ms / 1s / 5s / 10s
Low Pass Filter(V & A)	50KHz
Interface	RS-232

4015A List of Specification and applicable features

Model	4015A Power Meter With Harmonic			
No. of Input Channel	4			
Applicable test function				
1. Input RMS Current	4. No Load Power Consumption			
2. Input Frequency	5. Input Power Factor			
3. Input Power	6. Current Harmonic			
Specifications				
ACV meter (Vrms)	Range	15V / 0.001V, 30V / 0.001V, 50V / 0.01V 150V / 0.01V, 300V / 0.01V, 500V / 0.1V		
	Accuracy	±0.1% of (Reading + Range)		
ACA meter (Arms)	Range	20mA / 0.001mA, 500mA / 0.01mA, 10A / 1mA 50mA / 0.001mA, 2A / 0.1mA, 20A / 1mA 200mA / 0.01mA, 5A / 0.1mA, 200A peak / 0.01A		
	Accuracy	±0.1% of (Reading + Range)		
		±2% of (Reading + Range, for Inrush)		
ACW meter	Range	0.3W / 0.01mW 0.75W / 0.1mW 3W / 0.1mW 7.5W / 1mW 30W / 1mW 75W / 1mW 150W / 10mW 300W / 10mW	0.6W / 0.01mW 1.5W / 0.1mW 6W / 0.1mW 15W / 1mW 60W / 1mW 150W / 10mW 300W / 10mW 600W / 10mW	1W / 0.1mW 2.5W / 0.1mW 10W / 1mW 25W / 1mW 100W / 10mW 250W / 10mW 500W / 10mW 1000W / 0.1W
		3W / 0.1mW 7.5W / 1mW 30W / 1mW 75W / 10mW 300W / 10mW 750W / 10mW 1500W / 0.1W 3000W / 0.1W	6W / 0.1mW 15W / 1mW 60W / 1mW 150W / 10mW 600W / 10mW 1500W / 0.1W 3000W / 0.1W 6000W / 0.1W	10W / 1mW 25W / 1mW 100W / 10mW 250W / 10mW 1000W / 0.1W 2500W / 0.1W 5000W / 0.1W 10000W / 1W
		Accuracy ±0.1% of (Reading + Range)		
		Accuracy Same as AC		
		Accuracy Same as AC		
		Accuracy Same as AC		
		Accuracy Same as AC		
		Accuracy Same as AC		
PF meter	Range	±0.001~1.000 / 0.001		
	Accuracy	1% of (Reading + Range, Corresponds to V and A)		
Frequency meter	Range	40~70 / 0.1Hz		
	Accuracy	± 0.1 Hz		
V/A	Number	1~50 th / Same as ACV, ACA meter		
Harmonic	Accuracy	±0.5% of (Reading + Range)		
V/A THD	Range	0%~255% / 0.001%		
	Accuracy	±0.5% of (Reading + Range)		
Inrush Delay / Period		0~100ms		
Low Pass Filter(V & A)		50KHz		
Interface		RS-232		

4032-PD List of Specification and applicable features

Model	4032-PD Noise & Timing Analyzer Module		
Applicable test function			
1. Positive Voltage Transitions 2. Negative Voltage Transitions 3. Hard Reset 4. USB Type C Cable Unplug 5. Ripple Voltage 6. Dynamic Load Vpeak +/- Measure			7. Input Voltage Sag 8. Turn ON(Set-Up) Time 9. Turn OFF(Hold-Up) Time 10. Rise Time 11. Fall Time
Specifications			
No. of input channel	2		
Timing Measurement		Ripple Measurement	
Set-up / Hold-up / Rise / Fall Time		Band Width	0 ~ 100 KHz
Voltage range	0 ~ 10/30 Vdc	Voltage range	0 ~ 10 / 30 Vdc
Current range	*(1/4F.S.)/(F.S.) Adc	Measurement range	0 ~ 0.4 / 1 Vp-p
Timing range	1 Sec/2 Sec/4 Sec/8 Sec/16 Sec	Resolution	0.001 / 0.01V
Resolution	1 uS/2uS/4uS/8uS/16uS	Current range	*(1/4F.S.) / (F.S.) Adc
Vth1 / Vth2		Measurement range	*(1/8F.S.) / (1/2F.S.) Ap-p
Voltage range	5% ~ 95% of reading	Resolution	0.001/0.01A
Resolution	0.01V/0.01V, 0.001A/0.01A	Accuracy	±5% of (Reading + Range)
Accuracy	±2% of (Reading + Range)	Sampling Rate	100KHz
Noise Measurement		Update Rate	50~1000 mS
Low Pass Filter	up to 20 MHz	Resolution	1mS
Voltage range		Dimming Measurement	
Resolution	1mV	Band Width	100KHz
Accuracy	±2% OF reading + 5mV	Current range	*(1/8F.S.) / (1/2F.S.) Adc
Over Shoot Measurement		Resolution	0.001 / 0.01A
Band Width	0 ~ 100 KHz	Accuracy	±5% of (Reading + Range)
Voltage range	0 ~ 10 / 30 Vdc	Sampling Rate	100KHz
Measurement range	0 ~ 10 / 30 Vdc	Update Rate	50~1000 mS
Resolution	0.01 Vdc	Resolution	1mS
Current range	*(1/4F.S.) / (F.S.) Adc	Frequency range	10Hz~35KHz
Measurement range	*(1/4F.S.) / (F.S.) Adc	Resolution	1Hz
Resolution	0.001 / 0.01A	Accuracy	±1% of (Reading + Range)
Accuracy	±1% of (Reading + Range)	Duty(Ton) Range	3uS~90mS
Sampling Rate	100KHz	Resolution	1uS
Update Rate	50~1000 mS	Accuracy	±1% of (Reading + Range)
Resolution	1mS		
Vpeak Measurement		USB PD Timing Measurement	
Vpeak+/Vpeak-		PVT/NVP/Hard Reset/Output Voltage Falling Time	
Band Width	0 ~ 100 KHz	Va/Vb/Vc/Vd	
Voltage range	0 ~ 10 / 30 Vdc	Voltage range	0 ~ 10/30 Vdc
Measurement range	0 ~ 10 / 30 Vdc	Resolution	0.01 V
Resolution	0.01 Vdc	Accuracy	1% of (Reading + Range)
Accuracy	±1% of (Reading + Range)	Timing range	3 Sec
Sampling Rate	100KHz	Resolution	10 uS
Update Rate	50~1000 mS		
Resolution	1mS		

5303 AVR Suitable test item & Specifications

Model	5303 AVR
Suitable Test Item	
1. Input Inrush Current	
Specifications	
Power Rating	3KVA
Maximum Capacity	CF > 7
Input Voltage Rating	230Vrms +/- 10%
Output Voltage Rating	230,264,277Vrms Selectable
Accuracy	±2.5Vrms
Interface	RS-232 remote control only

PFR-100L/100M Suitable test item & Specifications

Model	Fanless Multi-Range D.C. Power Supply			
Suitable Test Item				
1. Over Voltage Protection				
Specifications	PFR-100L	PFR-100M		
Power Rating	100W			
Voltage range	0 ~ 50V	0 ~ 250V		
Resolution	40mV	200mV		
Current range	0 ~ 10A	0 ~ 2A		
Resolution	1mA	0.1mA		
Slew rate	Rise Time	50ms		
	Fall Time	100ms		
Protection		OCP , OTP		

99094-4 List of Specification and applicable features

Model	99094-4 Quick Charge Controller
Applicable test function	
1. USB PD Source / Sink Profile 2. USB PD Power Data Object (PDO) 3. USB PD Output Voltage Change 4. USB Type C Cable Unplug	
Specifications	
No. of Test Channel	4
Support Quick Charge	QC2.0, QC3.0, PE+, PE+2.0, USB PD
Terminal of Charger	D-sub 15Pin for ChxA, ChxB

Order Information



Basic version



Standard version



Value version



Complete version

6050-4-A1 (3332F)
USB PD 4 channel Test System

6050-4-B1 (3332F)
USB PD 4 channel Test System

6050-4-C1 (3332F)
USB PD 4 channel Test System

6050-4-D1 (3332F)
USB PD 4 channel Test System